




- V5: Flow cell drain
 V6: Flow cell fluid supply
 V10: BI sample tube OD flush
 V17: Sample air pressure to BI

 V7: BI load/unload
 V8: Accudrop filter IN/OUT
 V13: BI aspirator IN/OUT
 V15: Sort block aspirator IN/OUT
 V16: Laser shutter IN/OUT
 V14: R3 bypass for high pressure to BI

 V19: BI Aspirator Valve
 V20: Sample line back flush

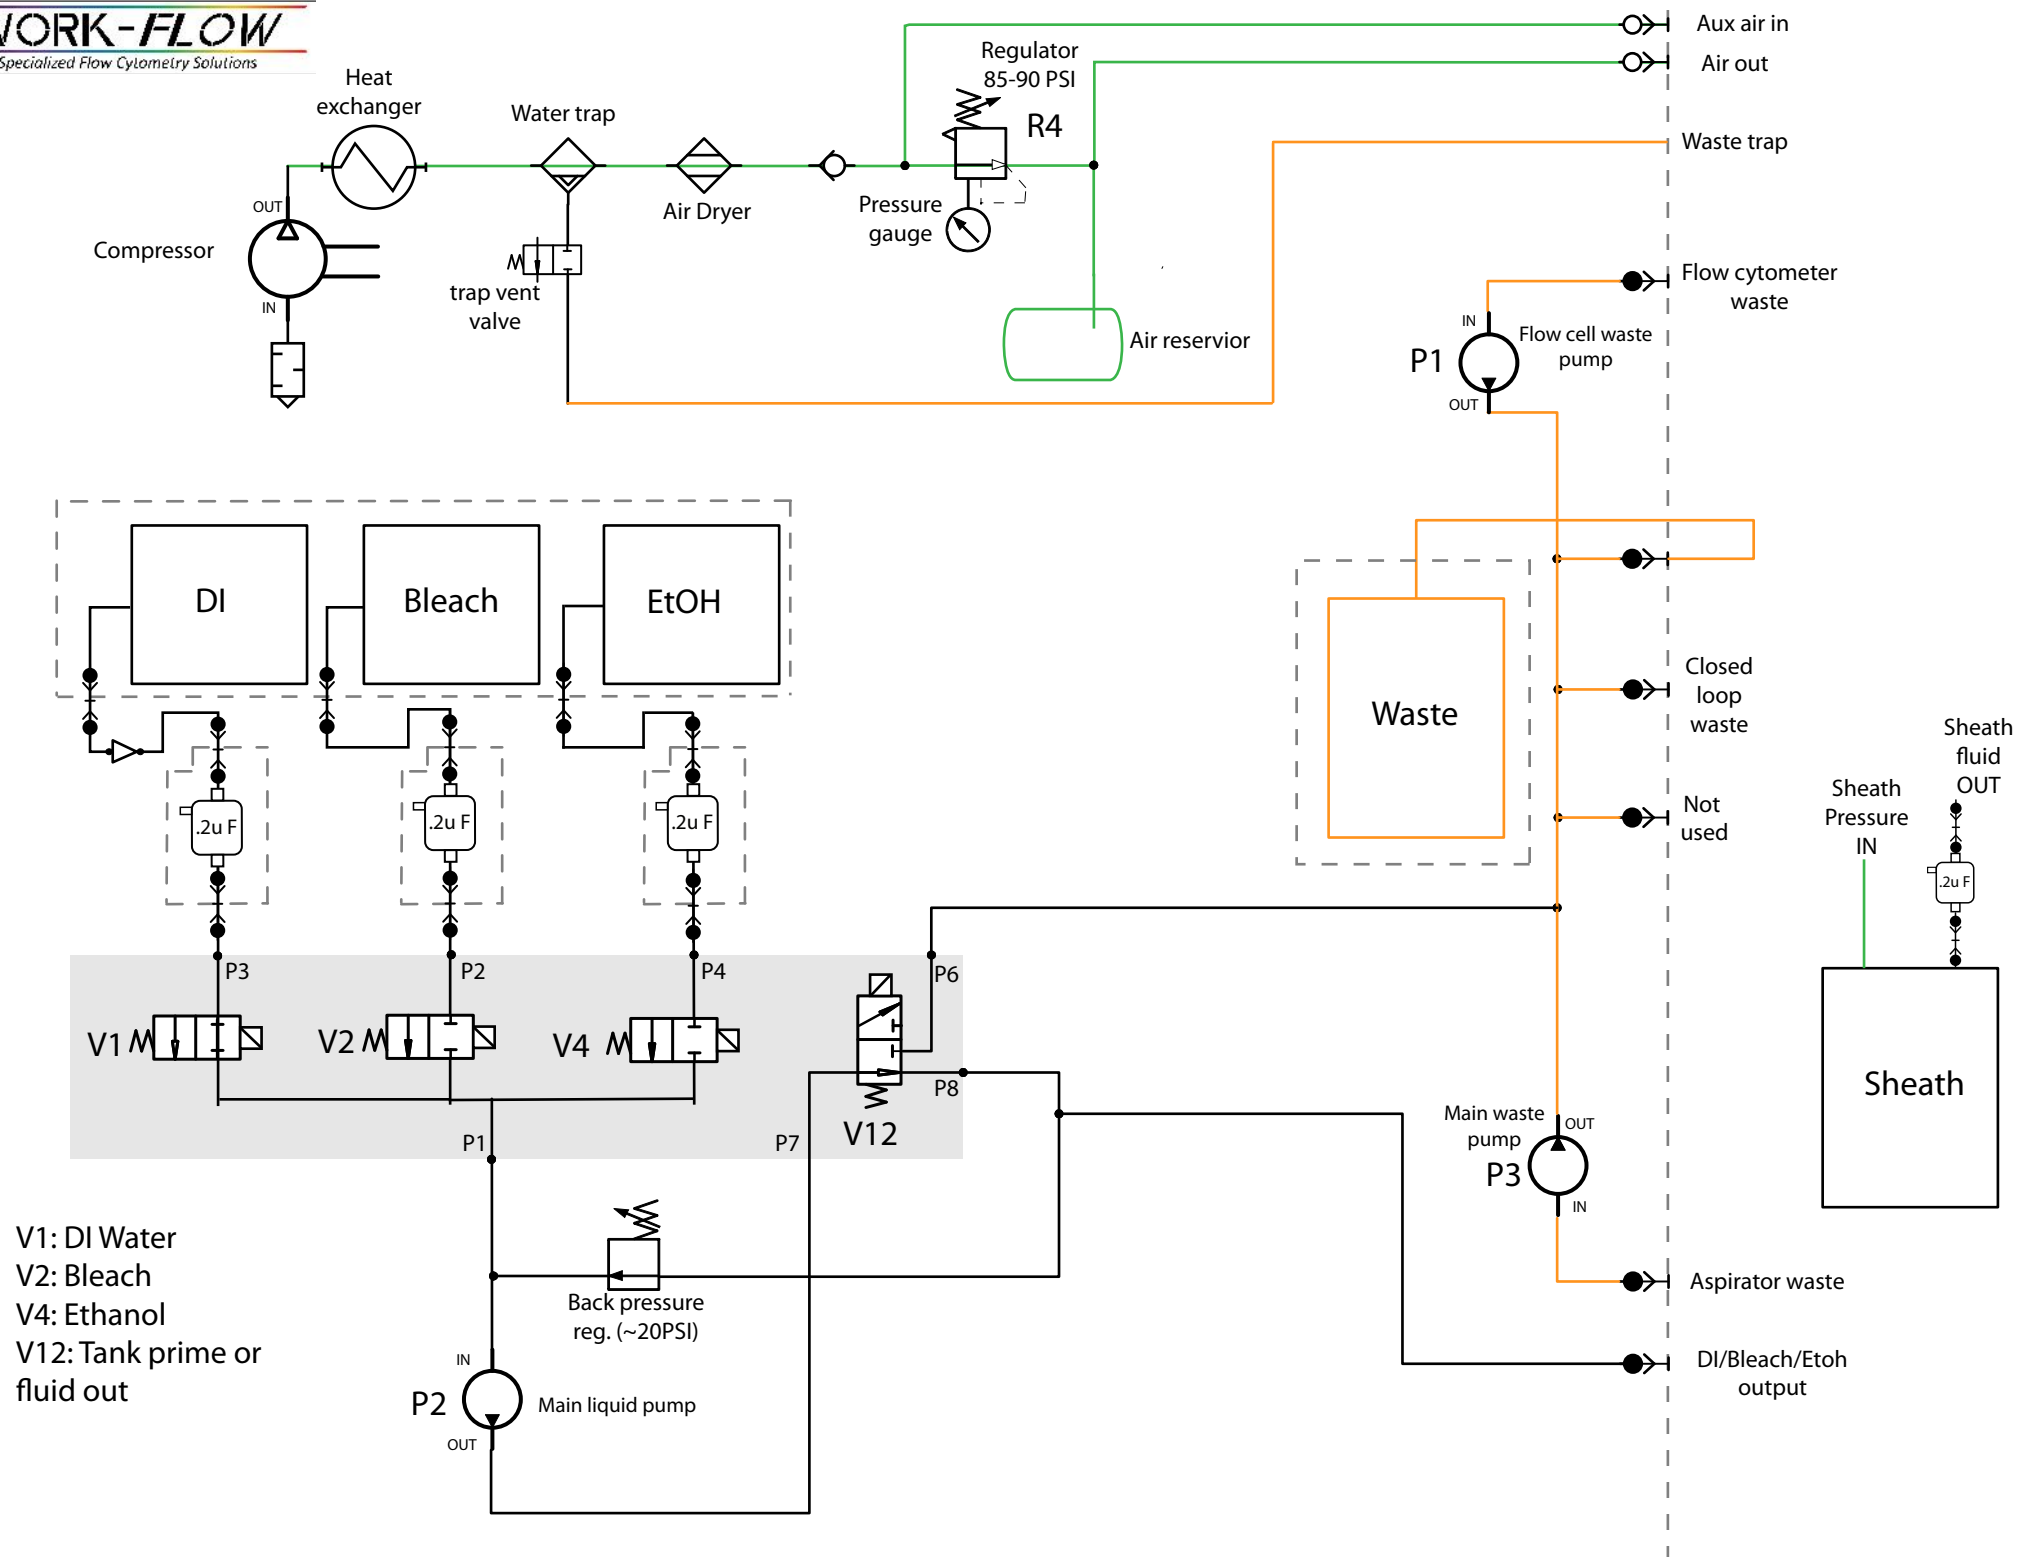